
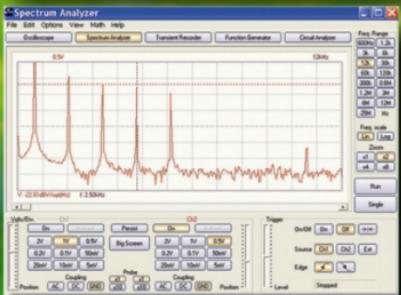


Pc-Lab 2000 SE™

GETTING STARTED / INSTRUCTIONS EN BREF / RATGEBER / INSTRUCCIONES BREVES

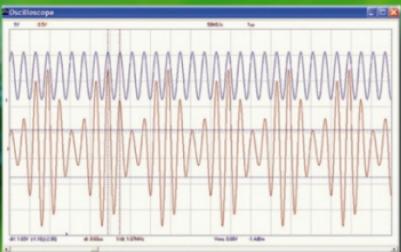

- PCS500 K8016/PCG10
- K8031/PCS100 K8047 / PCS10
- PCSU1000 PCGU1000

- OSCILLOSCOPE**
- SPECTRUM ANALYSER**
- TRANSIENT RECORDER**
- FUNCTION GENERATOR**
- BODE PLOTTER**

Amplitude:	CH1	CH2
<input checked="" type="checkbox"/> DC Mean	0.63 V	0.09 V
<input checked="" type="checkbox"/> Max	1.59 V	1.47 V
<input checked="" type="checkbox"/> Min	-0.28 V	-1.41 V
<input checked="" type="checkbox"/> Peak-to-Peak	1.88 V	2.88 V
<input checked="" type="checkbox"/> High	1.53 V	1.25 V
<input checked="" type="checkbox"/> Low	-0.22 V	-1.19 V
<input checked="" type="checkbox"/> Amplitude	1.75 V	2.44 V
<input checked="" type="checkbox"/> AC RMS	0.65 V	1.19 V
<input checked="" type="checkbox"/> AC dBV	-3.70 dBV	1.50 dBV
<input checked="" type="checkbox"/> AC dBm	-1.40 dBm	3.72 dBm
<input checked="" type="checkbox"/> AC-DC RMS	0.91 V	1.19 V
<input checked="" type="checkbox"/> AC-DC dBV	-0.704 dBV	1.59 dBV
<input checked="" type="checkbox"/> AC-DC dBm	1.43 dBm	3.72 dBm
Timing:		
<input checked="" type="checkbox"/> Duty Cycle	49.5 %	50.0 %
<input checked="" type="checkbox"/> Positive Width	1.19 ms	1.20 ms
<input checked="" type="checkbox"/> Negative Width	1.21 ms	1.20 ms
<input checked="" type="checkbox"/> Rise Time	0.688 ms	0.120 ms
<input checked="" type="checkbox"/> Fall Time	0.672 ms	0.104 ms
<input checked="" type="checkbox"/> Period	2.40 ms	2.40 ms
<input checked="" type="checkbox"/> Frequency	0.417 kHz	0.417 kHz
<input checked="" type="checkbox"/> Phase	19.9 deg	-19.9 deg
<input type="button" value="Select All"/>	<input type="button" value="Unselect All"/>	<input type="button" value="Close"/>
<input type="button" value="Help"/>		



velleman®
projects



www.velleman.be

<http://forum.velleman.be/>

English :

Hardware set-up.....	5
Install the software	6
Starting the software.....	7
The Oscilloscope	8
The Spectrum analyser.....	9
The Transient recorder	10
The Function generator	11
The 'More function'-button	11

Welcome to the world of Pc-Lab2000SE

This software can be used as an introduction to the powerful world of measuring, using the Velleman products.

The hardware is not necessary to evaluate the software in Demo mode.

This software can be used with the Velleman measurement instruments:

- **PCS500**, Dual channel digital storage oscilloscope, spectrum analyzer and transient recorder.
- **PCS100 / K8031** One channel digital storage oscilloscope, spectrum analyzer and transient recorder.
- **PCG10 / K8016** Pc function generator.
- **PCS10 / K8047** 4 channel recorder / logger.
- **PCSU1000** Dual channel USB PC oscilloscope, spectrum analyzer and transient recorder
- **PCGU1000** 2MHz USB Pc function generator.

Extra feature: Using the oscilloscope and generator on the same computer, this software creates the powerful bode -plot feature.

Hardware Set-up (Close all programs before continuing)

LPT connected devices (PCS500/PCS100/PCG10/K8016/K8031...):

- Connect your device using the supplied cable on a free LPT port
- Start the software after PC-LAB2000se installation (see next page)

USB connected devices:

PCS10 / K8047:

- Connect the PCS10 to a free USB port, a standard windows USB driver will be used.

(*) For Win98se an USB- HID driver update can be necessary (see CD).

PCSU1000 / PCGU1000:

- Connect your device to a free USB port
- Follow the on screen driver installation procedure.
- If Windows asks for Windows Update, select “not at this time”
- Install the driver from a specific location, then browse on the CD and select the folder **D:\PCSU1000_driver**. or **D:\PCGU1000_driver*** (press “next”)
- If Windows indicate “has not passed Windows logo testing...” select “Continue Anyway”.
- After finishing, you can check the driver installation in the Device Manager list. Under USB controllers “PCSU1000 oscilloscope” or “PCGU1000 should appear (only if unit is connected !).

(*) It is possible 2 drivers (USB and COM) must be installed by repeating the above.

For more information see the extended manual on the CD

* Microsoft Windows™ 98SE/ME/2000/NT4/XP/VISTA are registered trademarks

How to install **Pc-Lab2000SE**

Minimum system requirements :

- IBM compatible PC running Windows™ 98SE/ME/2000/XP/Vista (*).
- VGA display card (minimum 800x600, 1024x768 recommended)
- 10MB free hard disk space.
- Mouse or pointing device.
- CD or CD/DVD Rom player.
- Free parallel port for *PCS500 / PCS100 / PCG10 / K8016 / K8031*
- Free USB port (1.1 or 2.0) for *PCS10 / K8047 / PCSU1000 / PCGU1000*

Insert the **VELSOFT** CD into your drive.

If the “setup” does not start automatically, browse the CD and run the **SETUP.EXE** program.

Select “Install **Pc-Lab2000SE**”

An install wizard will guide you through the complete installation procedure. Shortcuts to the **Pc-Lab2000SE** software and the help files are automatically generated.



(*) **Note:** You will need local Administrator privileges to successfully complete the installation, contact your system administrator for assistance. See also the “ReadME” file in the installed folder.

* IBM, Microsoft Windows™ 98SE/ME/2000/NT4/XP/VISTA (*) are registered trademarks


Download the latest version from www.velleman.be and follow “downloads” link.

Starting the software :

Locate the **Pc-Lab2000SE** software shortcuts (programs.. *Pc-Lab2000SE ...*)

Click the icon  to start the main program.

- Select your connected hardware.
- Select your appropriate LPT port (if used).
- Press OK or choose “**demo mode**”.

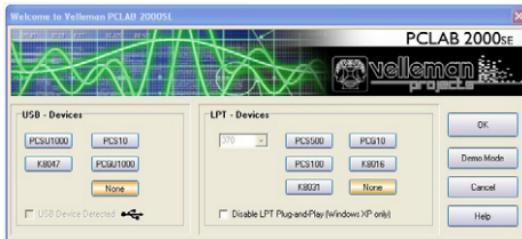

The main program automatically launches the Oscilloscope module, which is shown on the next page.

If you like to change the setup:

Click the **Options** menu, and select ‘**Hardware Setup**’.


Hint for LPT connected devices:

Should you experience troubles (e.g. When using a laptop or an oddball computer), try a different port address and/or choose the 'Slow' communication speed. Check also the port settings in the computer BIOS setting, test with the deferent settings; EPP (works in most cases), SPP, ECP... . For some Windows versions an additional I/O driver located on the CD could be needed.

REMARK: The actual screen can differ from the one shown in this manual. The PCS100 / K8031 has only 1 channel.

The main module featuring the Oscilloscope display :

What ? : The Oscilloscope module offers a feature-packed, easy to use digital storage oscilloscope.

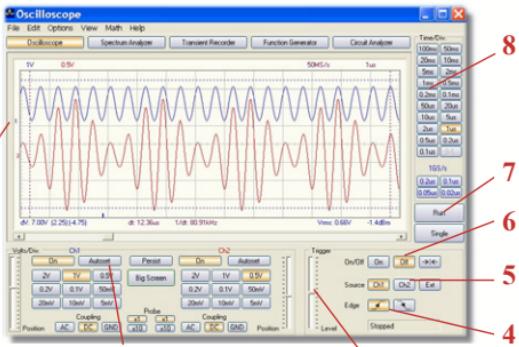

How ? :


- Connect the circuit under test to the scope input (observe the max. input rating of the scope!)
- Start measuring with “trigger off” (6)
- Press ‘RUN’ (7)
- Choose the desired channel and volts/div setting or press “Auto-set” (2) Autoset can not be used in 1GHz mode (PCS500 only).
- Choose the appropriate time/div setting (8)

To enable triggering :

- Select trigger channel (5)
- Select trigger edge (4)
- Set trigger to ‘ON’ (6)
- Set trigger level by sliding (3). The trigger mark is displayed on the left hand side of the signal display (1)

The Spectrum Analyser Module :

What ? : Powerful feature which allows visualization of the frequency spectrum of a signal, using FFT (Fast Fourier Transform) analysis.

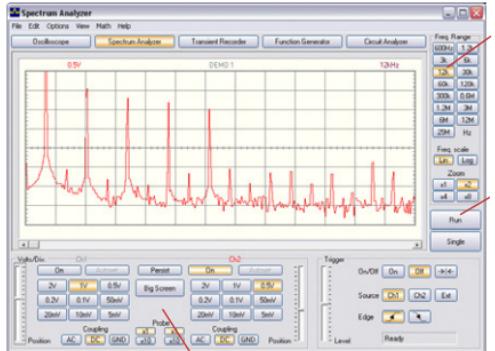


How ? :

- Connect the scope input to the circuit under test. (observe the max. input rating of the scope!)
- First observe the signal on the scope screen (see previous page).
- Check that the signal is not over the maximum of the screen.
- Start the spectrum analyzer.
- Press 'RUN' (1)
- Select the appropriate frequency range. Make sure your setting will capture any signal change of interest (3).
- If wanted set the appropriate channel and volts/div setting (2)

The Transient Recorder Module :

What ? : Record occasional events and log slow changing processes automatically, e.g. battery charge cycles, temperature changes,... or track intermittent faults in electronic circuits. Automatic data storage allows over one year of continuous recording !

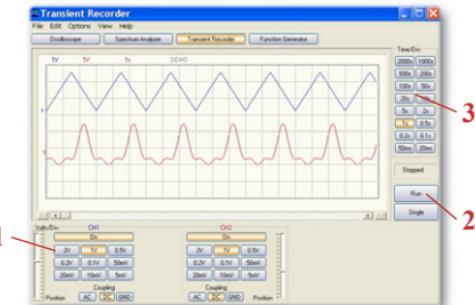

PCS500 / K8016 / PCG10 / K8031 / PCS100 / PCSU1000


How ? :

- Connect the scope input to the circuit under test.
 - Select the appropriate channel and volts/div (or volt range) setting (1).
 - Select the appropriate time/division setting (3).
 - Press RUN (2) to start recording.
- ☞ Press RUN again , to stop the measurement, or use the “Single” button to make a single screen measurement.


For continuous recording with auto-save to your HD, select ‘AutoSave Data’ from the ‘File’-menu.

Notes:

- ☞ During recording the screen can differ from the actual measurement.
- ☞ Events happening between two sample acquisitions will be missed if a too slow time/div is set

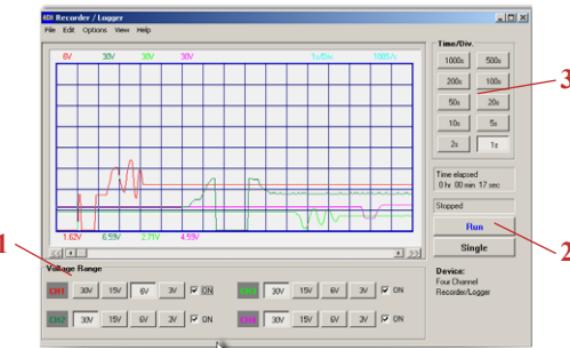


PCS10 / K8047

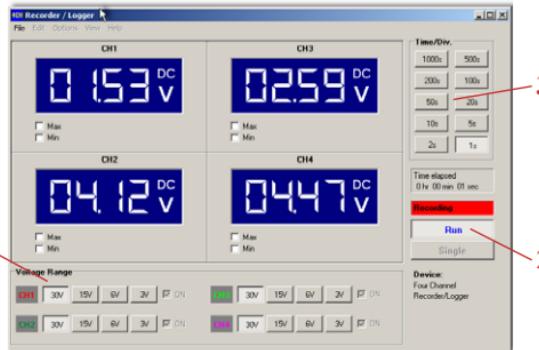

PCS10 / K8047

The Function Generator Module :

What ? : Most common waveforms are accessible at the touch of a button. A library with special functions is provided, as well as a Wave Editor, to create virtually any kind of waveform.

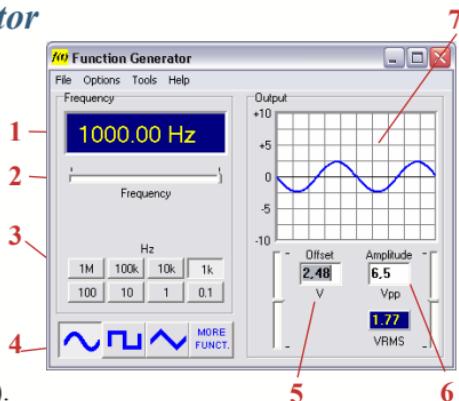


How ? :

- Click on the desired waveform (4).
- Select the desired frequency range (3).
- Set the exact frequency by sliding (2) or click the frequency readout (1) and enter a value.
- Adjust the offset (5)
- Adjust the amplitude (6)
(values can be entered by clicking the offset and amplitude readout)
- (7) shows a simulated preview of the output waveform

The ‘More Functions’- button :

The ‘More Functions’-button gives access to special purpose waveforms such as arbitrary waveforms, noise, frequency sweeps and DC. It also gives access to the waveform library.



More details can be found on the CD

Pc-Lab 2000 SE™

GETTING STARTED / INSTRUCTIONS EN BREF / RATGEBER /
INSTRUCCIONES BREVES

ELECTRONICS MADE EASY

4 CHANNEL RECORDER / LOGGER

K8047/PCS10■



TWO CHANNEL USB PC OSCILLOSCOPE

PCSU1000■



2MHz USB PC FUNCTION GENERATOR

PCGU1000■



K8016/PCG10■

0 TO 1MHz PC FUNCTION GENERATOR

Belgium [head office]	Velleman Components	+32(0)9 389 94 03
France	Velleman Electronique	+33(0)3 20 15 86 15
Netherlands	Velleman Components	+31(0)76 514 7563
USA	Velleman Inc.	+(877)785 - 7785
Spain	Velleman Components	95 412 68 00



velleman®
projects

www.velleman.eu